


DrySyn MULTI COOL Performance

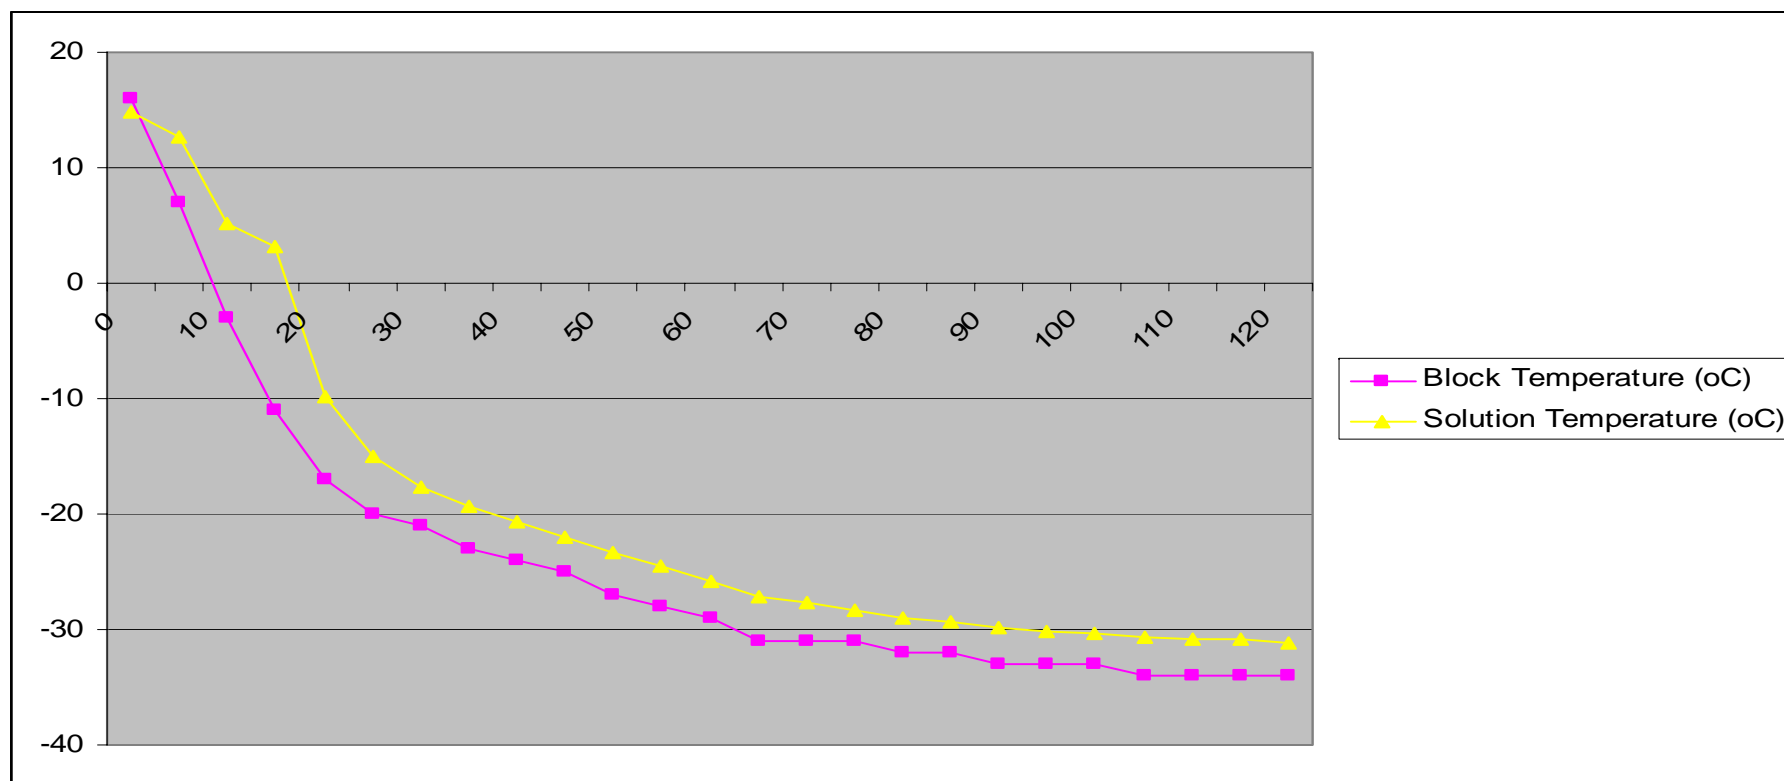

Testing was conducted using the following set up:

- Huber 240 Ministat Circulator with set point of -40C
- 2 x Insulated M16 hoses
- 2 x M16 adapters
- 5 Litres of -40 rated silicon oil
- DrySyn MULTI COOL Base
- 3 x 100 ml DrySyn COOL inserts
- 3 x 100 ml flasks (each with magnetic stirring bar & 50ml of silicon oil)
- Asynt ADS-HP1 hotplate stirrer set at 500rpm

No insulation was used